



Hb Control


Allow the control to stabilize for 30 minutes at room temperature before use.

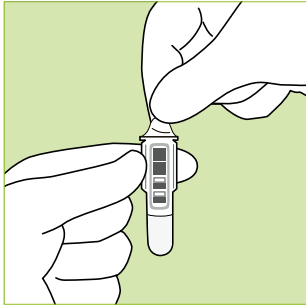



1 Remove the foil cover from the cuvette. Do not touch the clear flat surfaces in the lower part of the cuvette.

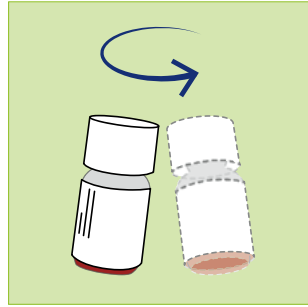


2 Mix the QuikRead go Hb 10 µl Control vial well. Do not shake. Red blood cells tend to sink to the bottom of the vial. Keep the bottleneck clean.

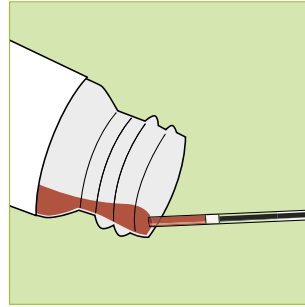


3 Tilt the control vial slightly. Place the capillary just below the control surface. Fill the orange striped capillary with the sample up to the white stopper. The control is stable for 5 minutes in the capillary.

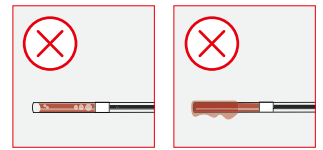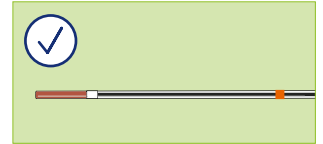


Note! Do not place the capillary to the bottom of the vial. If there are air bubbles on the capillary, discard it and collect a new sample. Wipe away any residual sample from the outside of the capillary.

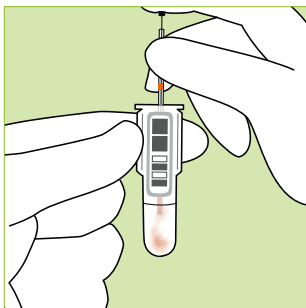


4 Place the sample (10 µl) into the buffer solution in the cuvette and dispense by pressing down the plunger. Make sure that the capillary is completely empty.

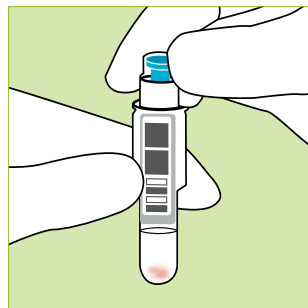

5 Close the cuvette tightly with the turquoise reagent cap. Do not press down the coloured inner part of the reagent cap. Perform the test within 2 hours.

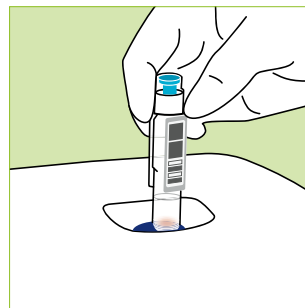

6 Choose "Quality Control" on the screen of the QuikRead go instrument. Insert the cuvette into the measurement well of the instrument. The barcode should be facing you.

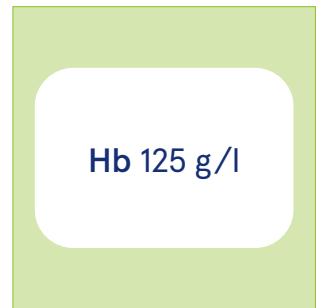

7 Measurement time is 2 minutes. The result is displayed on the screen, and the cuvette rises automatically when the measurement is completed. The acceptance limits of the control are in the labelling.

Storage

Opened vial is stable for 1 month at 2...8°C.

Note! Avoid using the last drops of the control.