



QuikRead go CRP


For QuikRead go Instrument and QuikRead go Plus Instrument

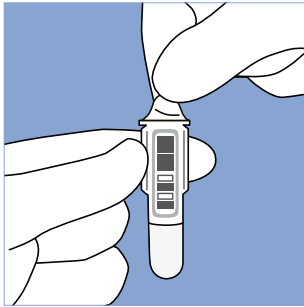


1 Remove the foil cover from the cuvette. Do not touch the clear flat surfaces in the lower part of the cuvette.

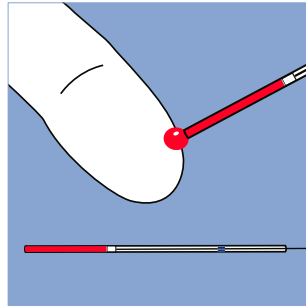


2 Fill the blue striped capillary with the sample (20 µl) up to the white stopper. Ensure that there are no air bubbles in the capillary. Wipe away any residual sample from the outside of the capillary.

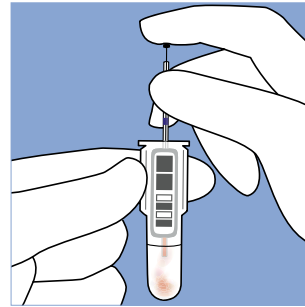


3 Place the sample (20 µl) into the buffer solution in the cuvette and dispense by pressing down the plunger. Make sure that the capillary is completely empty.

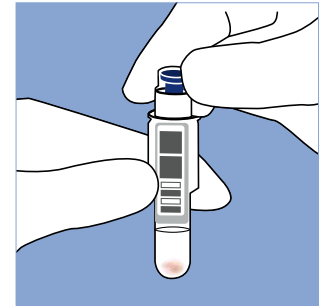

4 Close the cuvette tightly with the blue reagent cap. Do not press down the coloured inner part of the reagent cap. Perform the test within 2 hours.

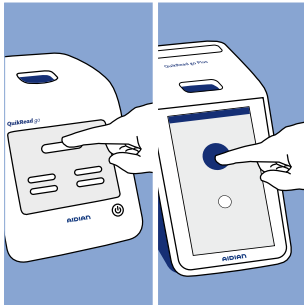

5 Choose Measure / Measure sample on the screen of the QuikRead go instrument.

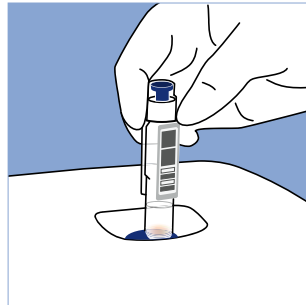


6 Insert the cuvette into the measurement well of the instrument. The barcode should be facing you.



7 Measurement time is 2 minutes. The result is displayed on the screen, and the cuvette rises automatically when the measurement is completed.

Please consult the instructions for use before performing the test.

QuikRead go CRP

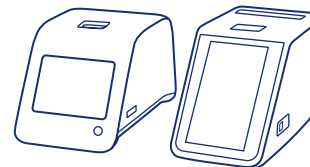

Kit

Unopened kit at 2–8°C: until the expiry date of the kit



Reagent cap tube

Storage at 2–8°C: until the expiry date of the kit
Storage at 18–25°C: 1 month (3 months when 7.5 hours/day)



Cuvettes

Unopened foil pouch at 2–25°C: until the expiry date of the kit
Unopened cuvettes after opening the foil pouch:
at 2–8°C: 6 months / at 18–25°C: 3 months



Opened cuvette

Let the buffer warm up to 18–25°C before testing
Perform the test within 2 hours from opening the cuvette
The sample is stable in the buffer for 2 hours



CRP controls

Unopened vial at 2–8°C: until the expiry date
Opened vial at 2–8°C: up to 2 months

Contact and orders

Aidian Oy, Finland

aidian@aidian.eu / +358 10 309 3000

orders@aidian.eu

quikread.com

Product	Cat. no.
QuikRead go CRP with capillaries and plungers	135171
QuikRead go CRP Control	153764
QuikRead go CRP Control High	153763
QuikRead Capillaries (20 µl)	67962
QuikRead Plungers	67966
QuikRead go Instrument	133893
QuikRead go Plus Instrument	155378