




# QuikRead go iFOBT

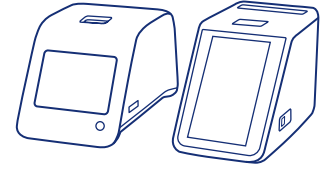


For QuikRead go Instrument and QuikRead go Plus Instrument

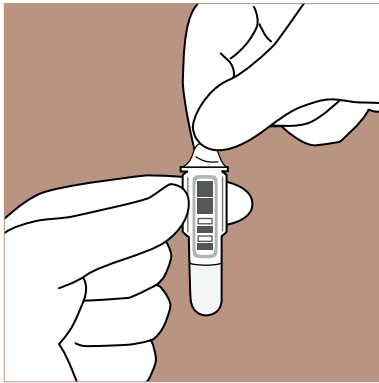


**1** Remove the foil cover from the cuvette. Do not touch the clear flat surfaces in the lower part of the cuvette.

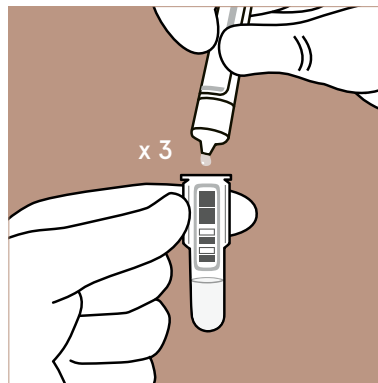


**2** Mix by inverting the sampling tube and break the tip. Discard the first three drops. Dispense the following three drops into the cuvette.

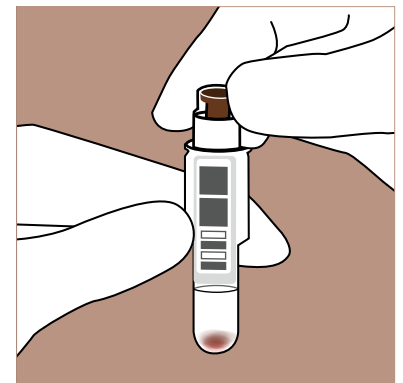

**3** Close the cuvette tightly with the FOB Reagent cap. Do not press down the brown inner part of the reagent cap. Perform the test within 2 hours.

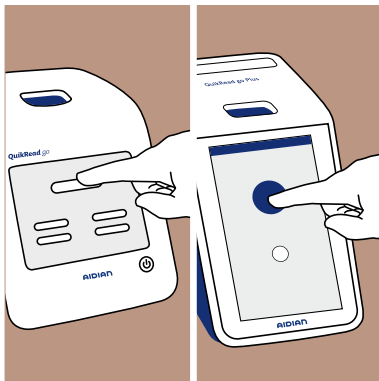

**4** Choose Measure / Measure sample on the screen of the QuikRead go instrument.

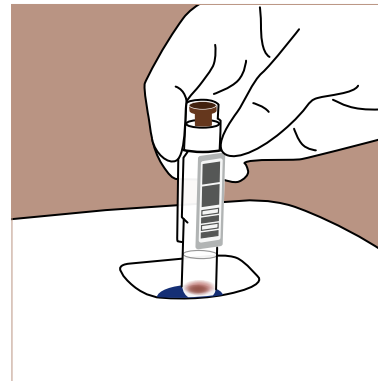


**5** Insert the cuvette into the measurement well of the instrument. The barcode should be facing you.



**6** Measurement time is 2 minutes. The result is displayed on the screen, and the cuvette rises automatically when the measurement is completed.

Please consult the instructions for use before performing the test.

# QuikRead go iFOBT

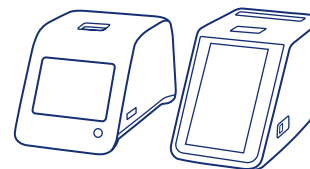

	Kit	Unopened kit at 2–8°C: until the <u>expiry date</u> of the kit
	Reagent cap tube	Storage at 2–8°C: until the <u>expiry date</u> of the kit Storage at 18–25°C: <u>1 month</u> (3 months when 8 hours/day)
	Cuvettes	Unopened foil pouch at 2–25°C: until the <u>expiry date</u> of the kit Unopened cuvettes after opening the foil pouch: at 2–8°C: <u>6 months</u> / at 18–25°C: <u>3 months</u>
	Opened cuvette	Let the buffer warm up to 18–25°C before testing Perform the test within <u>2 hours</u> from opening the cuvette The sample is stable in the buffer for <u>2 hours</u>
	QuikRead FOB Positive Control	Storage at 2–8°C: until the <u>expiry date</u>
	QuikRead go iFOBT Control Quantitative	Unopened vial at 2–8°C: until the <u>expiry date</u> Opened vial at 2–8°C: up to <u>1 month</u>
	QuikRead iFOB Sampling Set	Storage at 2–25°C: until the <u>expiry date</u> The sample is stable in the vial at 2–8°C for <u>7 days</u> or at 18–25°C for <u>5 days</u>

## Contact and orders

Aidian Oy, Finland

aidian@aidian.eu / +358 10 309 3000

orders@aidian.eu

quikread.com

Product	Cat. no.
QuikRead go iFOBT	151051
QuikRead FOB Positive Control	06027
QuikRead go iFOBT Control Quantitative	152390
QuikRead iFOB Sampling Set	151052
QuikRead go Instrument	133893
QuikRead go Plus Instrument	155378

8184-02EN, 01/2025. Not intended for the US market.  
The products are CE-marked either under IVDD (EC/98/79) or IVDR (2017/746).